


HEIGHT
ADJUSTABLE
ARMCHAIR WITH
THREE
ACTUATORS


INSTRUCTIONS FOR INSTALLATION, USE AND MAINTENANCE

3XL47



# **INDEX:**

-	EC declaration of conformity	1
-	Warranty certificate.	2
-	General provisions	3
	Presentation of the manual	
	Customer support service	
	Conventions	
-	Safety	4
	General provisions	
-	Introduction	5
	Technical presentation	
	Identification	6
-	General description	7
	Name of the parts	
	Technical features	8
	Materials used	9
	Functional check	10
	Disinfection	
	Assembly	11
-	Installation	12
	Transport and handling	
	Functional check	
	Operation and use	13
-	Maintenance	14
	Periodic verification	
	Provision and storage	15
	Scrappina	



# **EC** declaration of conformity

#### Released by:

We, undersigned CALDARA SRL with headquarters in VIA TRIESTE 31B – 22036 ERBA (CO), acting as manufacturer of the medical device:

Class I Medical Device (Non sterile),

#### 3XL47 - HEIGHT ADJUSTABLE ARMCHAIR WITH THREE ACTUATORS

Basic UDI-DI Code: 80551369202743XL47POLT

declares, under its own responsibility, that this medical device:

- complies with essential requirements and dispositions of Regulation (EU) 2017/745 (MDR)
- common Specifications have not been used for the compliance of the above medical device
- complies with directive 2011/65/EU (and subsequent amendments and integrations) on the restriction of the use of certain hazardous substances in electrical and electronic equipment

Single Registration Number (SRN): IT-MF-000036307

CALDARA S.T.I.

Erba, 15th November 2021

Claudio Febbi CEO at Caldara SRL

# Warranty certificate

This certificate must be kept until the expiry date.

It must be presented every time a technical intervention is necessary, accompanied by the invoice, tax receipt, delivery note or any supporting document showing the name of the retailer and the date of purchase.

The user who is unable to produce these documents will lose all the warranty rights.

The warranty starts from the date of purchase shown on the invoice, receipt or delivery note and it is valid for 24 months for the moving and electric parts, 36 months for the product structure.

The guarantee refers to the replacement or free repair, within the established terms, of the components of the appliance which, at the discretion of the manufacturer, were found to be defective at the origin due to manufacturing defects. This warranty does not cover:

- \_ transport faults (dents, scratches and similars);
- \_ damage due to falls;
- \_ damage caused by carelessness, negligence, inability to use the product, tampering and repairs carried out by unauthorized personnel;
- \_ damages due to incorrect installation; if this is carried out by the user or by unauthorized personnel;
- \_ damages caused by insufficiency or inadequacy of the electrical system or alterations deriving from environmental, climatic or other conditions, as well as damage caused by phenomena that do not depend on the normal operation of the appliance;
- \_technical interventions concerning the installation of the appliance and the connection to the power supply systems;
- \_ home repairs for convenience checks or alleged defects. If requested, the user will have to pay to the person in charge a contribution previously estimated in advance with the intervention;
- \_ordinary maintenance;
- \_whatever may be normal decay for use.

However, product replacement is excluded.

The warranty intervention can be refused when the product has been modified or transformed in any way. The restoration of the appliance will be carried out within the time limits compatible with the organizational requirements, by authorized technicians, upon request by the user to the retailer or directly to the manufacturer.

In the event of home intervention, the user is required to pay the fixed fee for transfer fees.

If the appliance is repaired at the retailer or at the manufacturer, the transport costs and the relative risks will be charged to the user.

Warranty repairs do not result in an extension of the warranty itself.

Parts replaced under warranty remain property of the manufacturer.

No one is authorized to change the terms and conditions of the warranty or to issue other verbal or written ones. The manufacturer declines all responsibility for any damage, of any nature, that may directly or indirectly derive from persons, animals or things resulting from failure to comply with all the instructions contained in this manual concerning, in particular, the installation warnings, use and maintenance of the appliance or in any case improper use.

The manufacturer is also not responsible for any damage caused to people, animals or things due to breakdown or forced suspension of use of the equipment. The Court of Como has jurisdiction for any dispute.

# **General provisions**

#### Presentation of the manual:

This manual is an integral part of the article.

Carefully read the warnings and instructions contained in this manual as they provide important information regarding SAFETY OF USE AND MAINTENANCE.

The descriptions and illustrations provided in this publication are not binding.

CALDARA S.R.L. reserves the right to make changes that it deems appropriate for the purpose of improvement, without committing to update this documentation.

The illustrations and images contained in this manual are intended as examples only and may differ from practical situations.

The manufacturer assumes no responsibility for direct or indirect damages, including loss of profits, or for any other damage of a commercial nature that may result from the use of the product that does not comply with what is described in this manual.

#### **Customer assistance service:**

Customer support and product support are important aspects of our corporate structure. We are at your complete disposal for further information on the use and maintenance of this product. (<a href="mailto:info@caldarasrl.it">info@caldarasrl.it</a>)

#### **Conventions:**

The following graphic symbols have been used in this manual:



WARNING! It is placed before certain procedures. Failure to comply may damage the

WARNING! It is placed before certain procedures. Failure to comply may damage the operator, the patient or the article.

# **Safety**

#### **General provisions:**



WARNING! Improper use and maintenance can cause damage to people and property.

WARNING! NOTICE FOR BLOOD DISEASES: to reduce the risk of exposure during the use of the chair, follow the maintenance instructions given in this manual, in addition to the provisions on the safety of personnel prepared by the head of the Emergency Medical Service.

Operators must carefully read this manual, follow the instructions it contains and become familiar with the correct procedures for using and maintaining the product.

Use and maintain the item only as prescribed in this manual and use only spare parts and assistance CALDARA S.R.L.

Keep this manual for consultation and in support of staff training.

Transfer it with the product in case of sale or transfer to new users.

### Introduction

#### **Technical presentation:**

The armchair is made of metal with remarkable performance characteristics that guarantee the structure stability and robustness. The very strong and resistant central column allows you to adjust the structure in height, its strength is equal to 4000N. The structure has excellent manoeuvrability determined by the use of 3 electric actuators controlled by a button panel.

The backrest is adjustable with an electric actuator and can reach  $+ 75^{\circ}$  positive and  $-8^{\circ}$  negative; the leg cushion also operated by an electric actuator reaches  $-90^{\circ}$  in negative and  $+5^{\circ}$  in positive. The armchair is equipped with a roll holder and has 4 adjustable feet which guarantee greater stability.

The base of the very compact structure allows the operator to get closer to the patient, making it very practical and comfortable. The upper surface and the armrests (cm 46 x 13,5) are in foam without seams, with high density; covered in fireproof class 1 IM coated fabric (skai, imitation leather). The spherical joint allows you to adjust the armrests with millimetric precision in any position and also to facilitate patient access they can be rotated in the backrest direction. The density of the rubber used guarantees the patient comfort and correct support during the visit.

The electrical parts comply with current hospital regulations.

#### **Reference standards**

The article was designed and built by CALDARA S.R.L. in compliance with the safety requisites foreseen by the directive (EU) 2017/745 (MDR) (class I) concerning medical devices.

#### Intended use

- \_Type of device: examination bed electrically height adjustable for examinations and therapeutic treatments in ambulatory and hospital environment. INDOOR USE.
- \_Environmental setting: hospitals and clinics in application environments 2 and 5. The room must be equipped with an electrical system in compliance with the regulations in force.
- \_ Staff assigned to use the product: specialized operators and doctors.
- \_ Supervision and responsibility: the bed must be used under the supervision of a doctor.
- \_Warning: the bed cannot be used in a potentially explosive atmosphere.
- \_Use limitations: the bed can only be used as described in this manual.

#### **Environmental limits of use**

The environmental conditions of use of the chair must follow these indications:

- \_Temperature: (0 to 50) C °
- \_Humidity: 10% -90% (not condensed)

#### **Expected life**

The bed has been designed to work without danger or risk to things or people, within the limits and conditions defined in this manual for a period of 10 years, after which replacement is recommended. Correct functioning is guaranteed only by contacting the manufacturer or retailer whenever a fault occurs and in accordance with the instructions contained in this manual.

#### Manufacturer

The article described in this manual is produced by:



CALDARA S.R.L. Via Trieste 31/B 22036 Erba (CO) Italy PH +39 031 640896 info@caldarasrl.it www.caldarasrl.it

#### **Identification:**



#### WARNING! it is forbidden to remove for any reason whatsoever label on the product.

The item can be identified by the label on the product following data is reported:

Name and address of the manufacturer

\_CE mark

\_Article model

\_Serial number



The electrical devices can be identified from the respective labels where the following data are reported:

#### **Column actuator:**

- Name and address of the manufacturer
- Article model
- \_Serial number
- Production date
- \_Maximum actuator load and IP protection degree
- \_Operation / consumption
- \_CE mark
- \_Production place
- \_Special waste



#### **Control unit:**

- Name and address of the manufacturer
- Article model
- \_Serial number
- \_Production date
- \_Functioning
- \_Max. Consumption
- \_IP protection degree
- \_CE mark
- \_Special waste




#### Applied part (control panel / perimeter / pedal board)

Class: Type B (Item Model / Serial Number)

#### **Control panel**



#### Perimeter



#### **Pedal board**




# **General description**

### **Component names:**

- 1\_Base
- 2\_Seat
- 3\_Headboard / backrest
- 4\_Columns
- 5\_Control panel
- 6\_Adjustable anatomical leg holders



### **Technical features:**

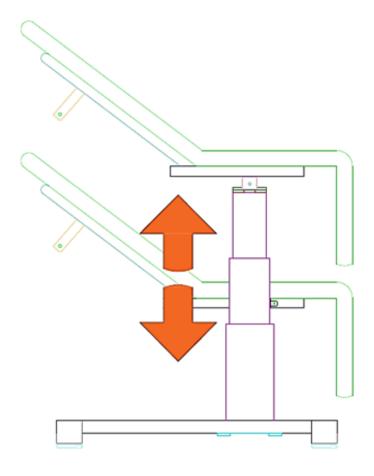

#### Materials used:

- \_Painted and galvanised steel for the metal structure;
  \_Top in wooden material, high density foam covered in fireproof washable class 1IM skai for the padded top;
- \_Column electric actuator with control unit and control devices for the adjustment of the upper surface;
- \_Gas spring for headboard adjustment;
- \_Galvanised steel bolts.

#### **Functional verification:**

WARNING! This check must be repeated periodically to verify the efficiency of the product.

Before using the product: perform the "periodic check" provided in the Maintenance chapter.

#### Sanitising:

WARNING! Use neutral non-corrosive products available on the market. Sanitising agents can be corrosive.

Carefully read the instructions provided by the manufacturer of the sanitising agent for the specific application.

It is very important to follow the specifications concerning concentration, temperature and reaction times; changing one of these characteristics can cause damage to the product and alter its characteristics. Depending on how the chair is used, the user will establish useful sanitation intervals.

Assembly:				
There are no parts to be assembl	ed.			
		11		

### Installation

#### **Transport and handling:**

WARNING! The lifting and handling operations must be carried out by specialized personnel trained in this type of operation.

It is necessary to use means suitable for the transport and handling of this product such as manual or self-propelled forklift trucks, taking care to respect the precautions and rules for safety at work.

The product must be installed and used in environments suitable for its use, away from any atmospheric agents capable of compromising its correct use and functioning.

At the time of delivery or collection it is necessary to check that the contents are intact and that the equipment made for its use is also complete; only after carrying out these checks is it possible to eliminate the packaging in disposal and collection places of the recycled material.

If the item is damaged during transport, retain the packaging and contact the carrier within 48 hours of delivery.

#### **Functional verification:**

WARNING! This check must be repeated periodically to verify the efficiency of the product.

Before using the product:

perform the "periodic check" provided in the Maintenance chapter.

If the check fails, contact your dealer or CALDARA SRL and take the chair out of service;

in case of a positive result, use the product after observing the points described above.

#### **Operation and use:**


- 1\_Place the bed on a flat non-yielding floor.
- 2\_the space surrounding the bed must be free and allow for adjustment and maintenance operations.

WARNING! always before seating the patient if the product is equipped with wheels, check that they are locked or raised from the ground.

WARNING! the power cable must be adequately protected and must not hinder the operator.

WARNING! When moving the bed, it is necessary to check that you have unplugged the power cord from the wall socket; re-evaluating the previous points.

- 3\_Seat the patient with the upper surface in a horizontal position and not in the tr / rtr position.
- 4\_Use one of the supplied controls to adjust the upper surface.

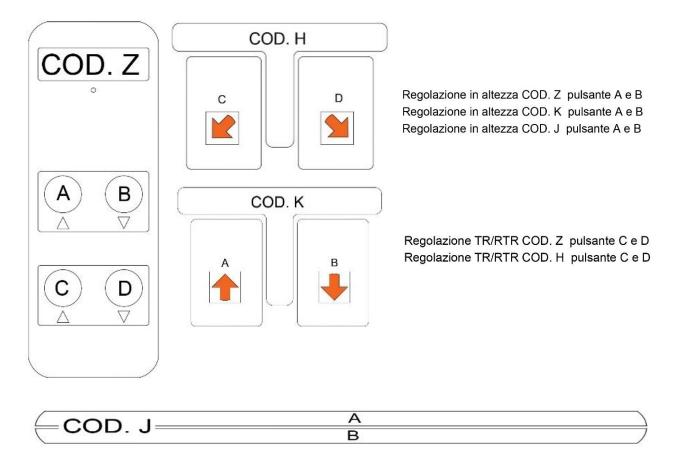

## **Maintenance**

#### Periodic check:

It is necessary to inspect the product at least once a year.

An inspection means a visual search for any damage that could compromise the integrity and proper functioning of the article. You must check:

- \_ integrity of the power cord and plugs;
- \_ correct power cable connection;
- \_tightening of screws;
- \_ correct functionality;
- \_correct insertion of any accessories.

WARNING! If damage is detected, immediately place the product out of service until it is repaired and put back into service.

WARNING! Any repairs and efficiency improvements are advised to be carried out by specialized technical personnel of the sales or assistance service.

#### Cleaning:

we recommend an accurate and periodic general cleaning of the product for a longer and better duration.

WARNING! It is recommended NOT to use: thinners, alcohol or petrol, aggressive and abrasive detergents.

Use water and neutral soap, rinse with a damp cloth and dry completely. This is an operation to be performed when necessary or at least every 15 days.

#### **Shelving or storage:**

In the event of provision or storage, the following instructions must be followed:
\_pack the product;
\_position it on a flat and safe surface;
\_must be in a dry place and away from the sun;
\_grease the moving parts which could be damaged in case of drying;
\_do not overlap any other item to the one set aside or stored.

#### **Scrapping:**

In case you decide not to use this product anymore, you need to: \_ make it inoperative;

\_make any parts that could cause dangers harmless.

In the event that this product is to be scrapped, it is necessary:

- \_evaluate the classification of the asset according to the degree of disposal;
- \_separate the various components and place them in the appropriate collection centres;
- \_if considered special waste, dispose of according to the laws in force.







**CALDARA SRL** – VIA TRIESTE 31B – 22036 ERBA (CO) ITALY – TEL/PH +39 031 640896 – P.IVA 01456450137